Certificate of Analysis


Bio-Analysis Centre

Oil Distributors Ltd

Blend 2: CJC1295No DAC + Ipamorelin

Analysis Method:

Sample Preparation	Dissolved in water (2ml)			
Instrument	Shimadzu Nexera HPLC	Injection Volume	5µl	
Column	Zorbax Extend C18	Analysis wavelength	215nm	
Column Dimensions	4.6 x 150 mm	Run time	30 mins	
Guard Column	Yes	Gradient	Time (min)	%B
Mobile Phase A	0.1% Formic Acid in Water		0 - 0.5	2
Mobile Phase B	0.1% Formic Acid in Acetonitrile		0.5 - 20.5	2 - 30
Flow	1 ml/min		20.5 - 20.6	30 - 95
Column Temperature	40°C		20.6 - 25.5	95
Autosampler temperature	15°C		25.5 - 25.7	95 - 2

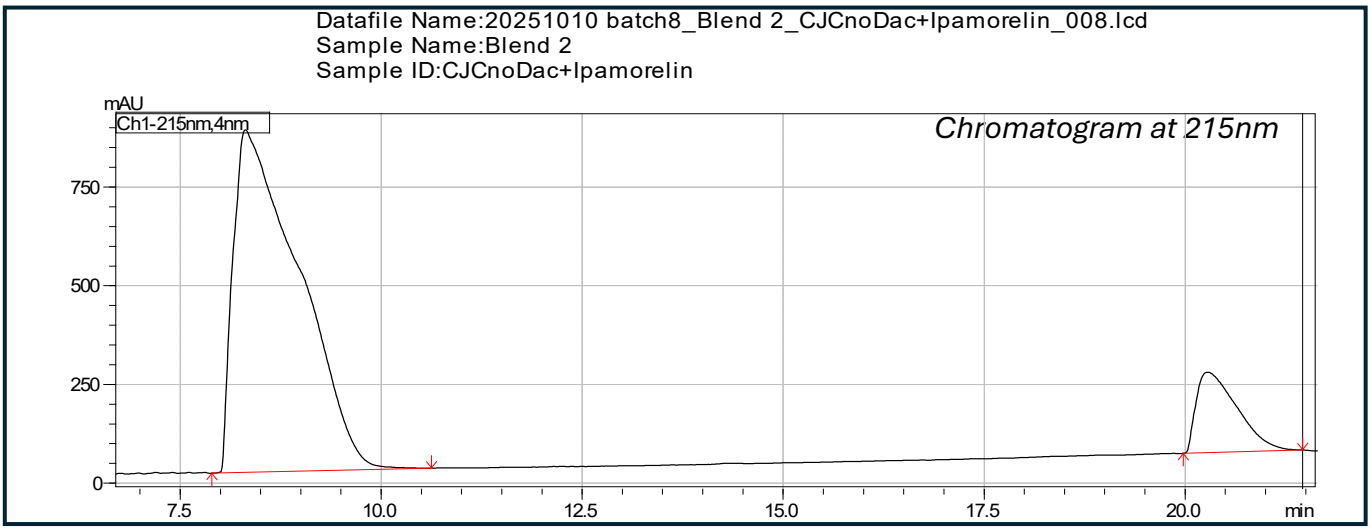

Peak Table

Peak#	Ret. Time	Area	Area%	Peak Purity Index	% Purity
1	8.309	49297040	87.27	0.99621	99.62
2	20.27	7188987	12.73	0.98414	98.41

Peak Purity Graph

