
Certificate of Analysis

Oil Distributors Ltd
HGH

Bio-Analysis Centre

Analysis Method:

Sample Preparation	Dissolved in water (3ml)			
Instrument	Shimadzu Nexera HPLC	Injection Volume	1µl	
Column	Kinetex C8	Analysis wavelength	215nm	
Column Dimensions	4.6 x 150 mm	Run time	15 mins	
Guard Column	No	Gradient	Time (min)	%B
Mobile Phase A	0.1% Formic Acid in Water		0 - 0.5	20
Mobile Phase B	0.1% Formic Acid in Acetonitrile		0.5 - 10.5	20 - 60
Flow	1 ml/min		10.5 - 12.6	60
Column Temperature	40°C		12.6 - 12.7	60 - 20
Autosampler temperature	15°C			

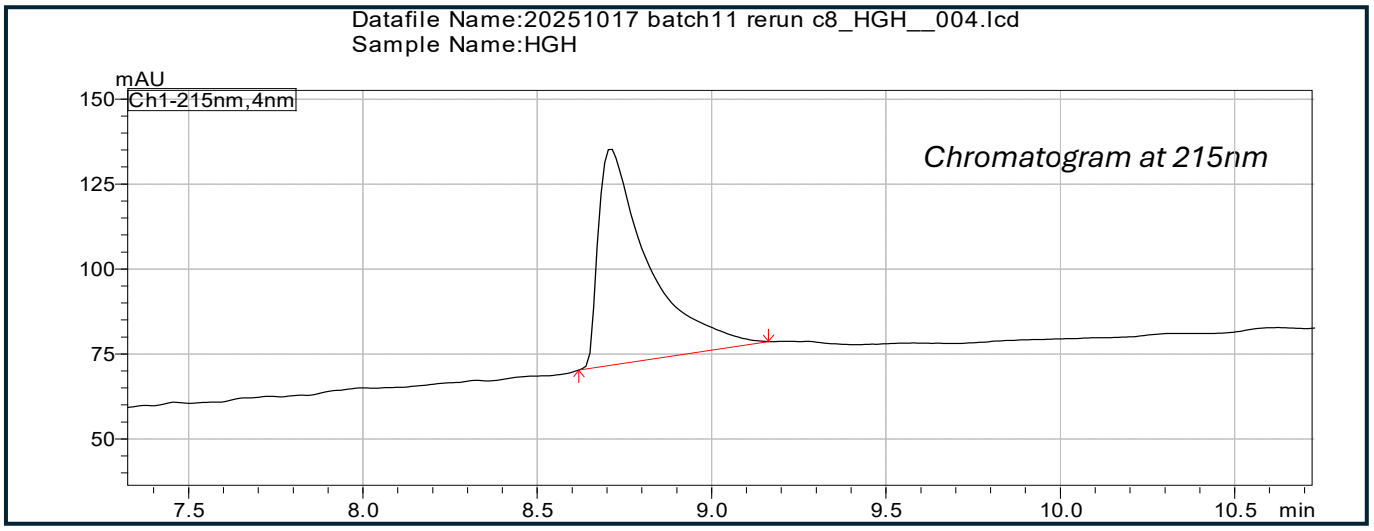

Peak Table

Peak#	Ret. Time	Area	Area%	Peak Purity Index
1	8.704	635932	100	0.99265

Overall Purity *99.3*%

Peak Purity Graph

